
SMARTMOUNT

Mouting Bracket for e-Series Ventilators


01.SETTING UP

Remove from packaging. Ensure all components are in place as per Fig. 1.

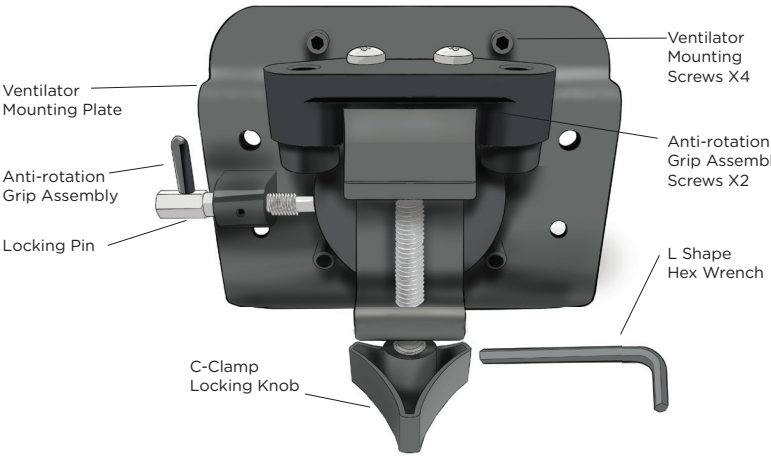

02. Attachment of e-Series Ventilators to the Mounting Bracket


Attach Ventilator to “SMART MOUNT” Mounting Bracket (Fig 2.) using the L Shape Hex Wrench provided. Tighten 4 ventilator mounting screws firmly. (Do not overtighten)

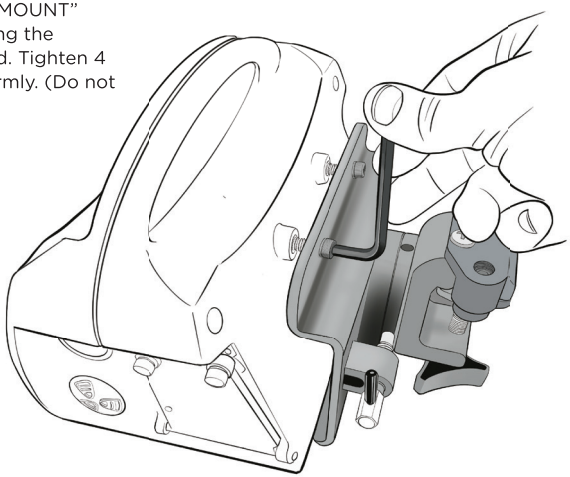

03. Mounting SMART MOUNT

A Mounting Bracket to Stretcher Bar or I.V. Pole. Ensure that the pole or bar is clean and free from oil or grease. The pole/bar diameter should be between 0.5" - 1.25".

B For first time attachment, attach the Smart Mount C-Clamp to the selected mounting location and tighten the C-Clamp locking knob (Fig 3).

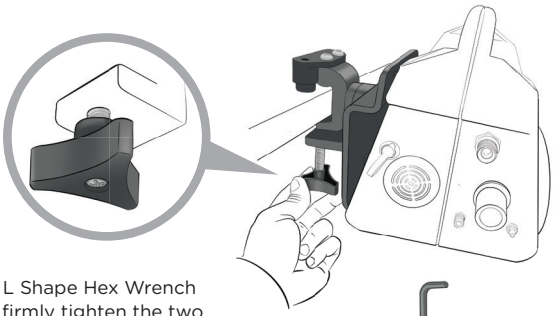

C Using the L Shape Hex Wrench provided, firmly tighten the two anti-rotation grip assembly screws to the mounting bar, I.V. pole or other location (Fig 4).



D Check the C-Clamp locking knob for a tight fit and retighten if necessary.

E The ventilator may now be attached and removed from the same mounting bar, I.V. pole or other location by using the C-Clamp locking knob only.

NOTE

When mounting to the same diameter mounting bar, I.V. pole or other location in the future the initial set up detailed in steps 3 and 4 will not be required. If mounting to a mounting bar, I.V. pole or other location of different diameter please repeat steps 1 through 4.

CAUTION

- Pole diameter 12.5 mm - 30 mm max. (0.5 - 1.2 in).
- Ensure clamp and pole are clean from oil or grease.
- Frequently inspect clamp and ventilator attachment screws to ensure they are correctly tightened.